



US009872604B2

(12) **United States Patent**  
**Kucklick et al.**

(10) **Patent No.:** **US 9,872,604 B2**  
(45) **Date of Patent:** **\*Jan. 23, 2018**

(54) **ATRAUMATIC ARTHROSCOPIC INSTRUMENT SHEATH AND METHOD**

(71) Applicant: **Cannuflow, Inc.**, Campbell, CA (US)

(72) Inventors: **Theodore R. Kucklick**, Campbell, CA (US); **Martin Trieb**, Cloverdale, CA (US)

(73) Assignee: **Cannuflow, Inc.**, Campbell, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 204 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **14/979,246**

(22) Filed: **Dec. 22, 2015**

(65) **Prior Publication Data**

US 2016/0106301 A1 Apr. 21, 2016

**Related U.S. Application Data**

(63) Continuation of application No. 14/312,411, filed on Jun. 23, 2014, now Pat. No. 9,216,270, which is a continuation of application No. 13/211,144, filed on Aug. 16, 2011, now Pat. No. 8,758,227, which is a continuation of application No. 12/194,309, filed on Aug. 19, 2008, now Pat. No. 7,998,061, which is a continuation of application No. 10/769,629, filed on Jan. 29, 2004, now Pat. No. 7,413,542.

(51) **Int. Cl.**

**A61B 1/012** (2006.01)  
**A61B 1/317** (2006.01)  
**A61B 1/00** (2006.01)  
**A61M 1/00** (2006.01)

**A61M 25/06** (2006.01)  
**A61B 17/34** (2006.01)

(52) **U.S. Cl.**

CPC ..... **A61B 1/00135** (2013.01); **A61B 1/0014** (2013.01); **A61B 1/00082** (2013.01); **A61B 1/00154** (2013.01); **A61B 1/012** (2013.01); **A61B 1/317** (2013.01); **A61B 17/3415** (2013.01); **A61M 1/0084** (2013.01); **A61M 25/0662** (2013.01); **A61B 2017/349** (2013.01)

(58) **Field of Classification Search**

CPC ..... **A61B 1/00135**; **A61B 1/00082**; **A61B 1/00154**; **A61B 1/00105**; **A61B 1/00121**; **A61B 1/012**; **A61B 1/317**; **A61B 17/3415**; **A61M 1/0084**; **A61M 25/0662**; **A61M 2025/0681**

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,156,142 A \* 10/1992 Anaplotis ..... A61B 1/00135  
600/156  
5,339,800 A \* 8/1994 Wiita ..... A61B 1/00091  
600/109

(Continued)


*Primary Examiner* — John P Leubecker

(74) *Attorney, Agent, or Firm* — K. David Crockett, Esq.; Susan L. Crockett, Esq.; Crockett & Crockett, PC

(57) **ABSTRACT**

A removable, resilient atraumatic sheath for arthroscopic instruments. The sheath covers sharp edges on the arthroscopic instrument, particularly the distal tip of the rigid cannula, and thereby protects tissue and objects near a surgical site from accidental trauma. The sheath may be provided in the form of an inflow/outflow sheath that allows a surgeon to irrigate and drain a surgical field without the use of a separate irrigation instrument.

**18 Claims, 5 Drawing Sheets**

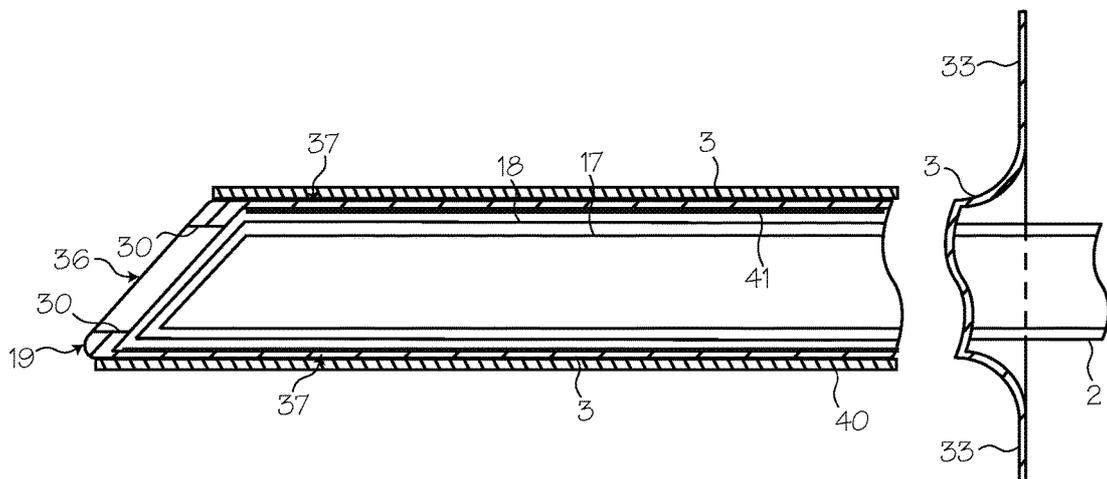


(56)




**References Cited**



U.S. PATENT DOCUMENTS


5,400,767 A \* 3/1995 Murdoch ..... A61B 1/00135  
600/157  
5,575,756 A \* 11/1996 Karasawa ..... A61B 1/00068  
600/121  
5,601,603 A \* 2/1997 Illi ..... A61B 17/0057  
604/12  
5,637,075 A \* 6/1997 Kikawada ..... A61B 1/00142  
600/105  
5,695,448 A \* 12/1997 Kimura ..... A61B 1/0005  
600/114  
5,697,888 A \* 12/1997 Kobayashi ..... A61B 1/00068  
137/606  
5,989,183 A \* 11/1999 Reisdorf ..... A61B 1/00091  
600/121  
6,086,542 A \* 7/2000 Glowa ..... A61B 1/317  
600/140  
6,354,992 B1 \* 3/2002 Kato ..... A61B 1/121  
600/157  
6,599,237 B1 \* 7/2003 Singh ..... A61B 1/0008  
600/114  
7,258,120 B2 \* 8/2007 Melker ..... A61M 16/04  
128/207.14  
2002/0069893 A1 \* 6/2002 Kawazoe ..... A61B 1/122  
134/1  
2003/0130565 A1 \* 7/2003 Muller ..... A61B 1/00071  
600/156  
2004/0082915 A1 \* 4/2004 Kadan ..... A61B 1/00068  
604/164.04  
2005/0085695 A1 \* 4/2005 Shener ..... A61B 1/00071  
600/156  
2005/0203341 A1 \* 9/2005 Welker ..... A61B 1/012  
600/130



\* cited by examiner

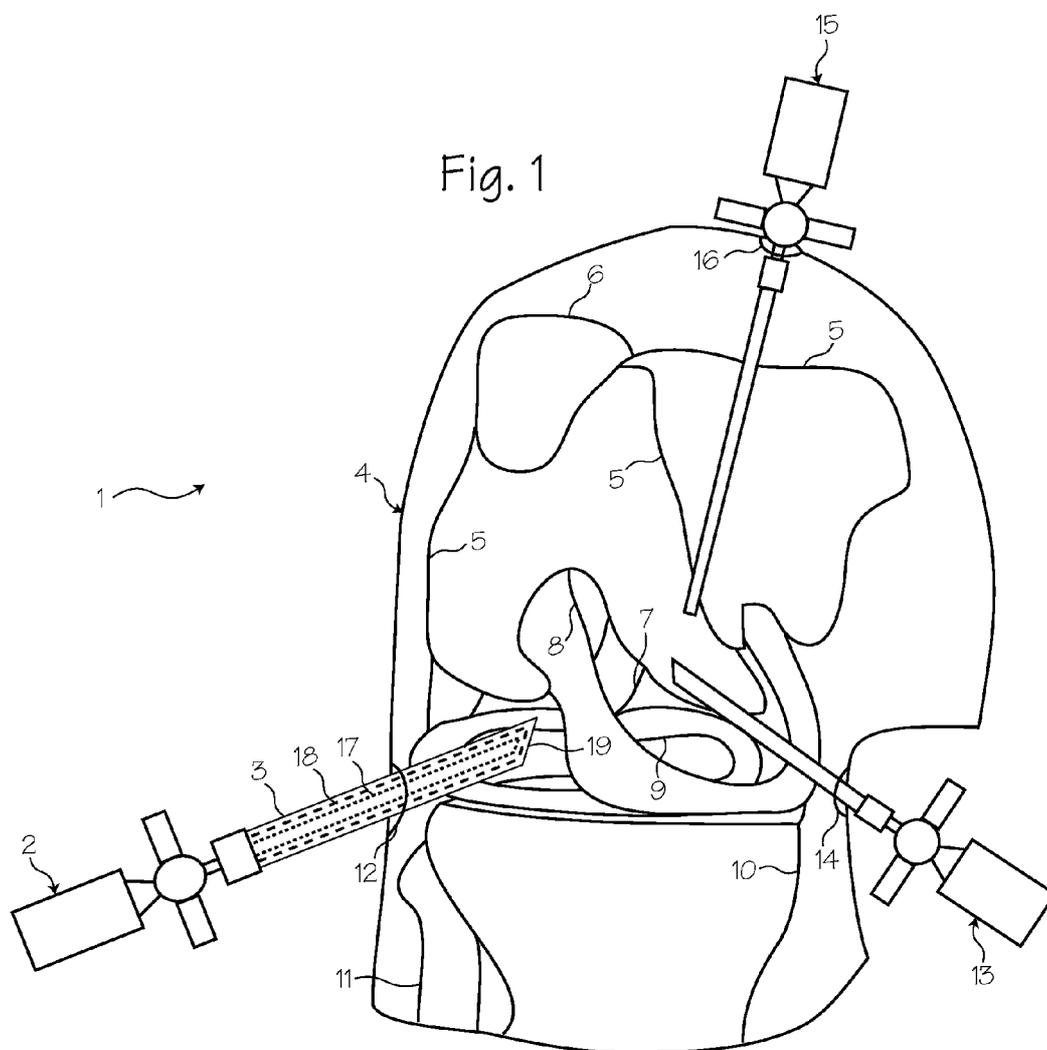

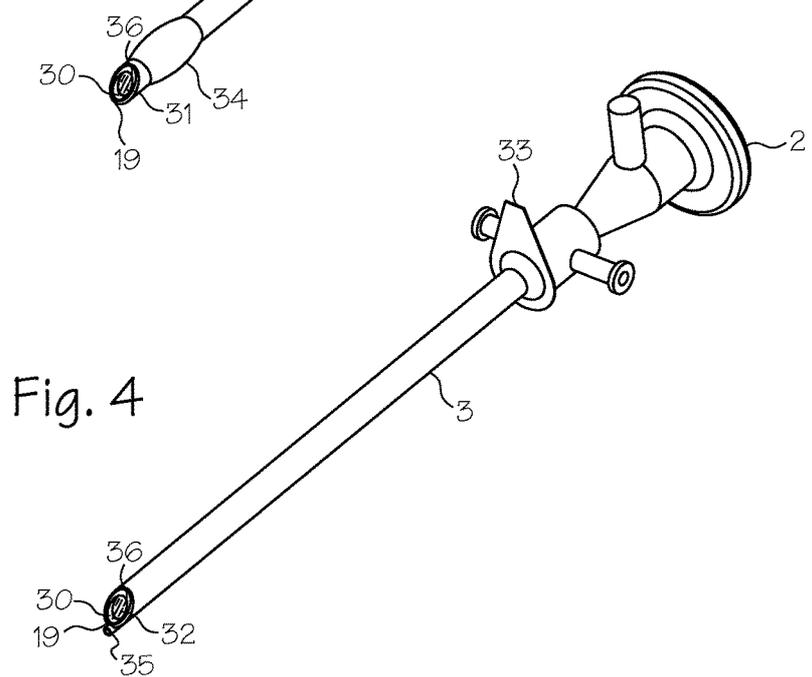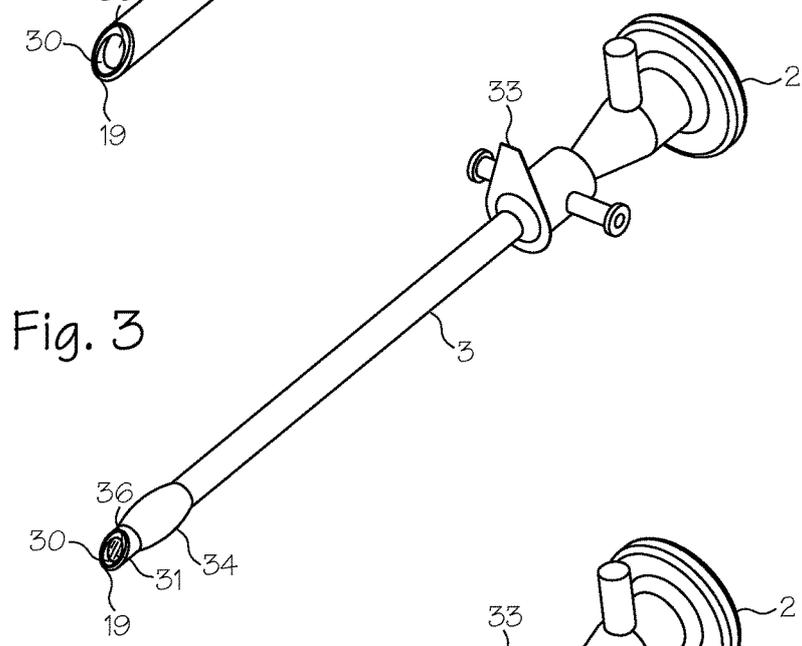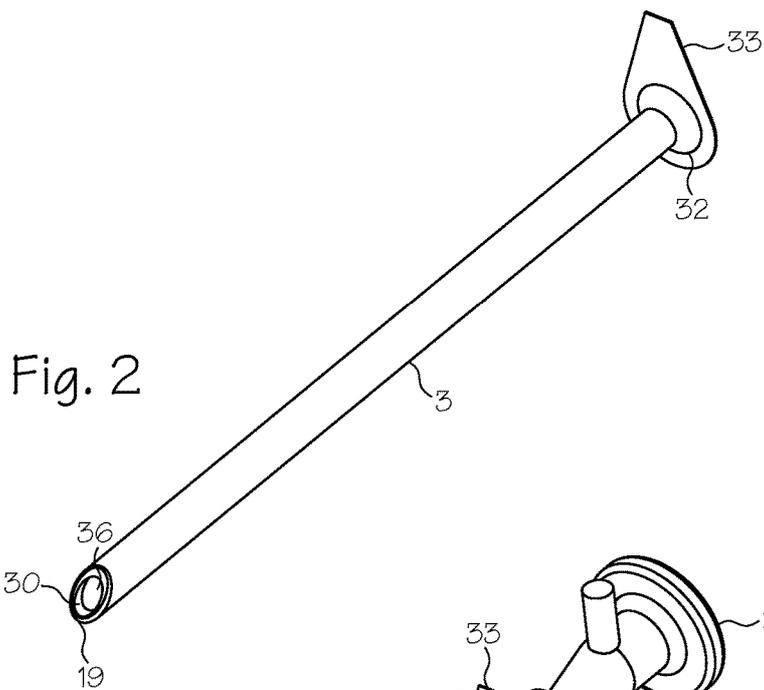

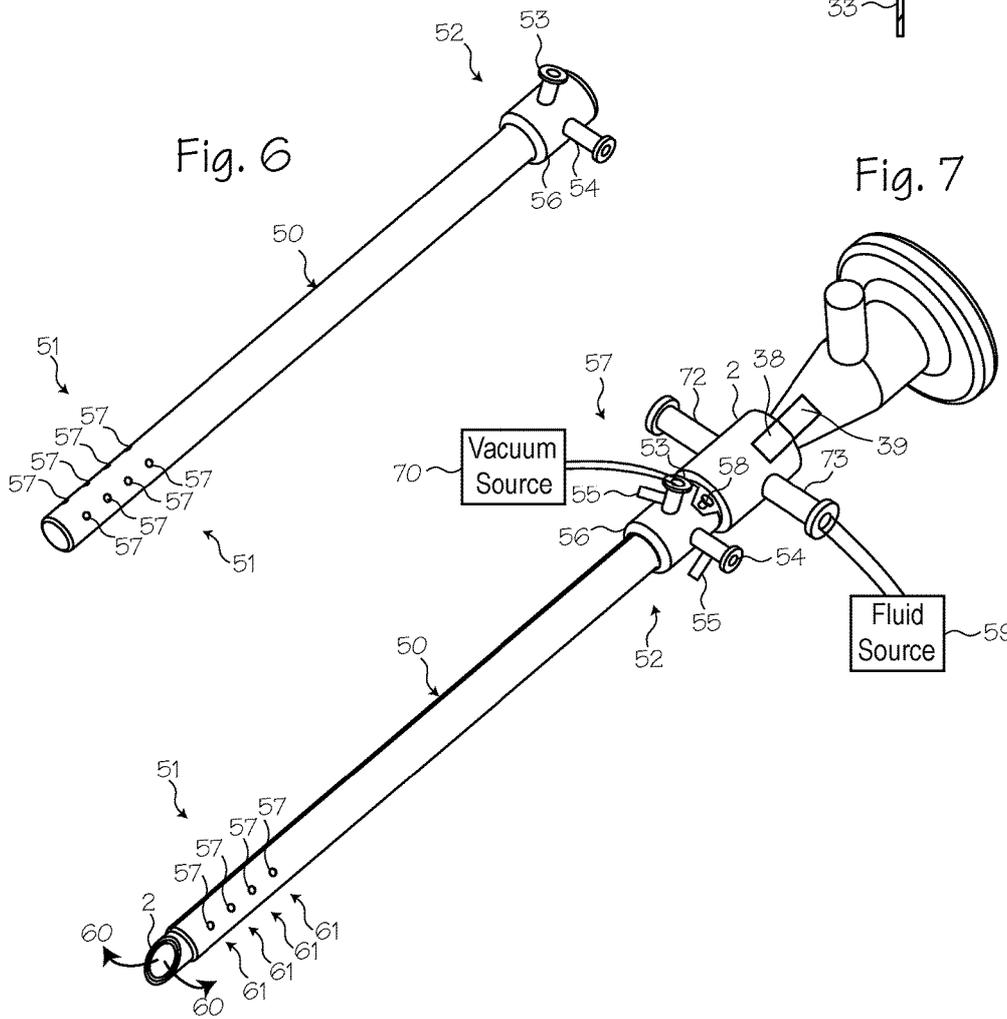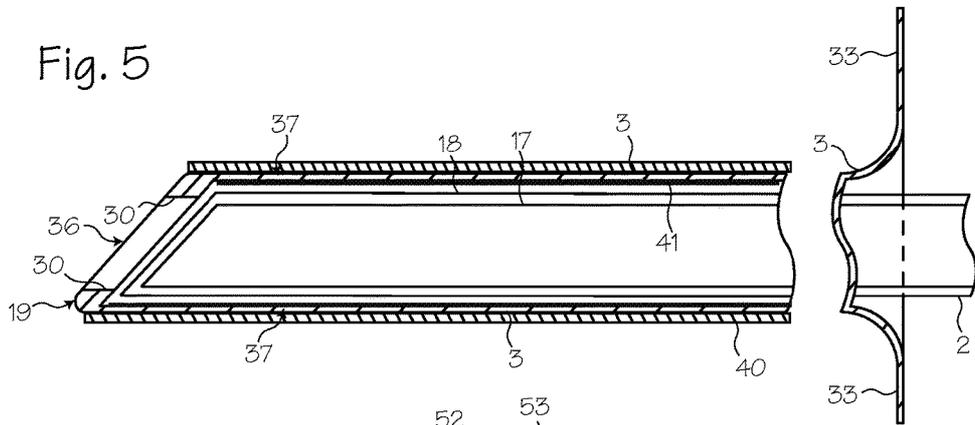

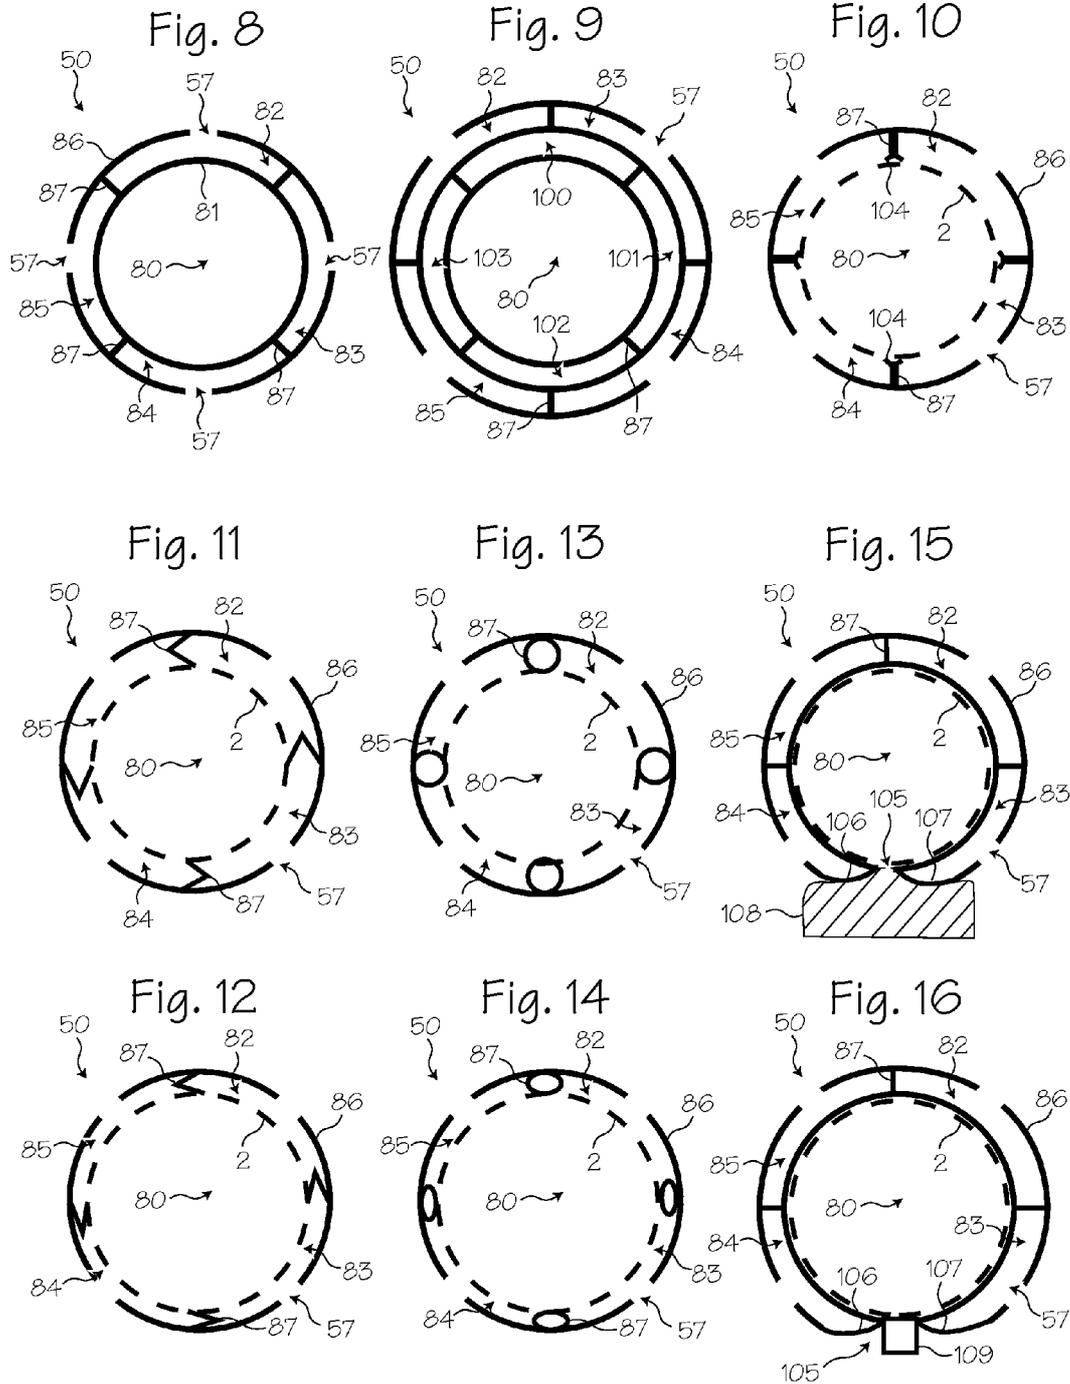

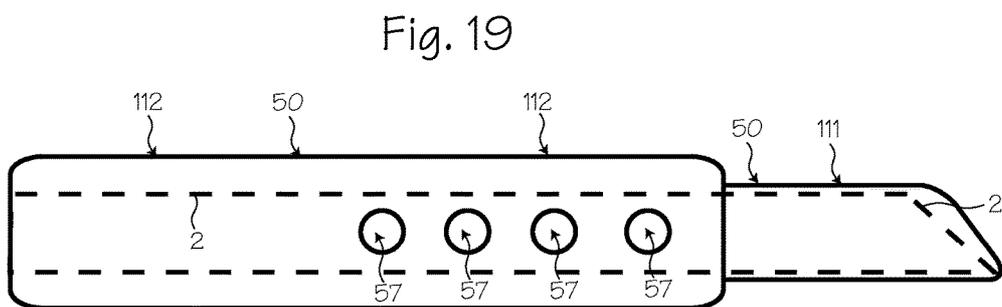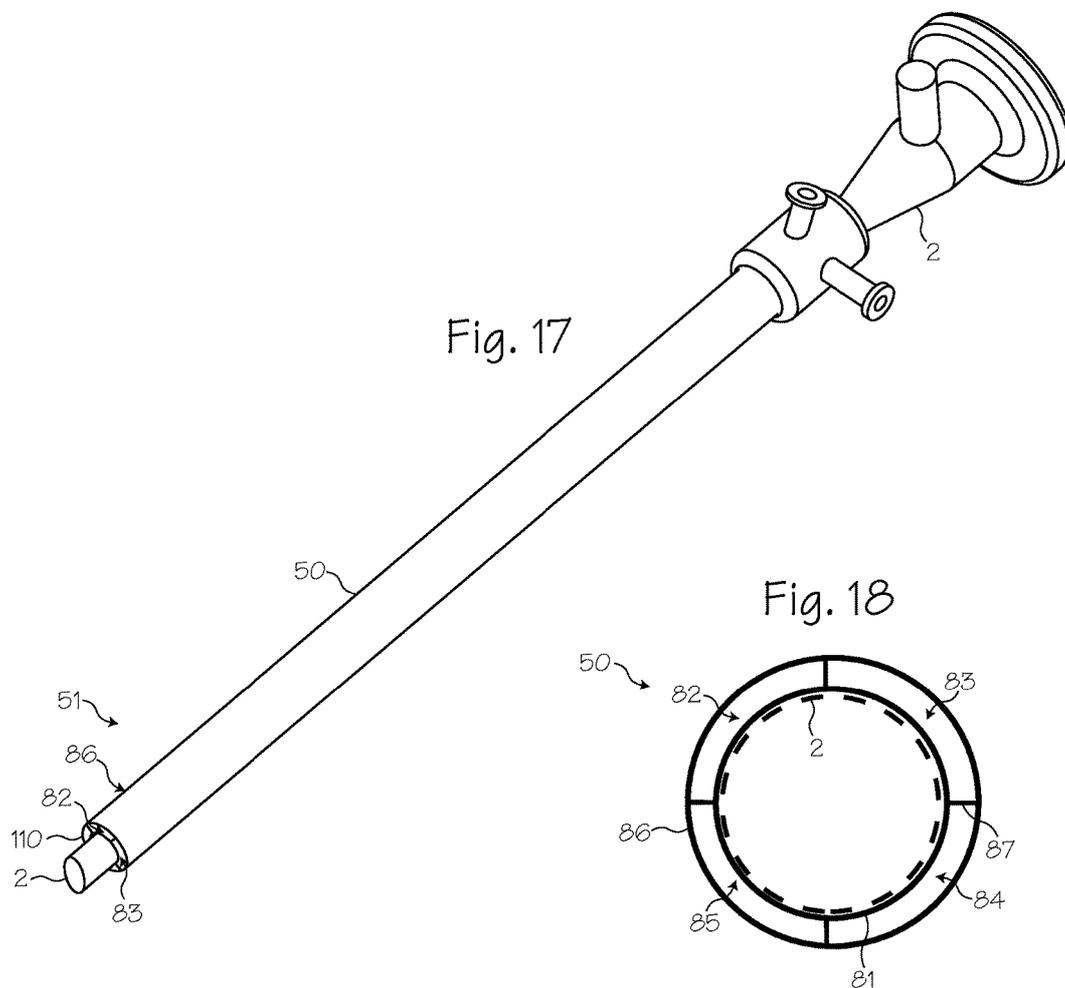

1

## ATRAUMATIC ARTHROSCOPIC INSTRUMENT SHEATH AND METHOD

This application is a continuation of U.S. application Ser. No. 14/312,411 filed Jun. 23, 2014, now U.S. Pat. No. 9,216,270, which is a continuation of Ser. No. 13/211,144 filed Aug. 16, 2011, now U.S. Pat. No. 8,758,227, which is a continuation of Ser. No. 12/194,309 filed Aug. 19, 2008, now U.S. Pat. No. 7,998,061, which is a continuation of Ser. No. 10/769,629, filed Jan. 29, 2004, now U.S. Pat. No. 7,413,542.

### FIELD OF THE INVENTIONS

The inventions described below relate the field of arthroscopic surgical instruments.

### BACKGROUND OF THE INVENTIONS

Arthroscopic surgery involves using optical instruments, such as an arthroscope, to visualize an operating field inside or near a joint of a patient. The same instrument or other instruments may be used to perform a surgical procedure in the operating field. Common instruments used in addition to the arthroscope include a trimming instrument for cutting tissue and an irrigation instrument for irrigating the surgical field. Each of the instruments requires its own incision to be introduced into the surgical field; thus, many surgeons prefer to use only a trimming instrument and an arthroscope during arthroscopic surgical procedures.

Arthroscopes are fragile in relation to the forces applied during arthroscopic surgery, so a rigid cannula is placed over the arthroscope to reinforce it. The distal end of the rigid cannula is pointed, usually sharp, and so the rigid cannula can scratch or gouge soft tissue within the operating field. The rigid cannula can also become stuck between bones or cartilage during a procedure. A rigid cannula can also damage metal prosthetics used to replace joints, resulting in a shortening of the useful life of the prosthetic and forcing the patient to undergo additional, painful surgeries to correct the problem.

An additional problem associated with arthroscopic surgery is maintaining a clear surgical field during surgery. Blood and debris can cloud the field, impairing a surgeon's ability to visualize tissue. One method of solving this problem is to use the irrigation instrument to clear the surgical field with saline; however, many surgeons strongly prefer to avoid the additional trauma caused by inserting a third instrument. These surgeons will perform arthroscopic surgeries despite problems with visualizing the surgical field. Thus, devices and methods are needed both to maintain a clear surgical field and reduce accidental injury to the patient while only using two instruments.

### SUMMARY

The devices and methods shown below provide for a soft plastic, disposable atraumatic sheath that slides over the rigid cannula of an arthroscope. The distal end of the atraumatic sheath extends slightly past the distal end of the rigid cannula, thereby providing a soft, blunt cushion over the distal end of the rigid cannula. The atraumatic sheath thereby protects any surrounding tissue or objects from accidental injury or damage while the arthroscope is manipulated inside the operating field.

The atraumatic sheath may also be provided as an inflow/outflow sheath that allows a surgeon to drain fluids from or

2

introduce fluids into the surgical field, thereby keeping the surgical field clear. The inflow/outflow sheath is a multi-lumen tube into which the arthroscope is inserted. The proximal portion of the sheath is provided with fluid ports, a manifold and other means of controlling the flow of fluid inside the sheath. The distal portion of the inflow/outflow sheath is provided with a plurality of holes. Each hole communicates with one or more of the lumens inside the tube, thereby allowing fluid to flow between the surgical field and sources or sinks located outside the patient. The inflow/outflow sheath thereby allows the surgeon to maintain a clear surgical field and protect the patient from accidental injury while eliminating the need for a third irrigation instrument.

### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 shows a method of performing arthroscopic surgery on a patient.

FIG. 2 shows an atraumatic sheath for use with arthroscopic instruments.

FIG. 3 shows an atraumatic sheath for use with arthroscopic instruments and an arthroscope disposed inside the atraumatic sheath.

FIG. 4 shows an atraumatic sheath for use with arthroscopic instruments, an arthroscope disposed inside the atraumatic sheath and an irrigation tube disposed on the sheath.

FIG. 5 shows a cross section of the atraumatic sheath shown in FIG. 2 and an arthroscopic instrument disposed inside the atraumatic sheath.

FIG. 6 shows an inflow/outflow atraumatic sheath for use with arthroscopic instruments.

FIG. 7 shows an inflow/outflow atraumatic sheath for use with arthroscopic instruments and an arthroscope disposed inside the atraumatic sheath.

FIG. 8 shows a cross section of the distal portion of the inflow/outflow atraumatic sheath of FIG. 7.

FIG. 9 shows a cross section of the distal portion of an inflow/outflow atraumatic sheath.

FIG. 10 shows a cross section of the distal portion of an inflow/outflow atraumatic sheath.

FIG. 11 shows a cross section of the distal portion of an inflow/outflow atraumatic sheath.

FIG. 12 shows a cross section of the distal portion of an inflow/outflow atraumatic sheath.

FIG. 13 shows a cross section of the distal portion of an inflow/outflow atraumatic sheath.

FIG. 14 shows a cross section of the distal portion of an inflow/outflow atraumatic sheath.

FIG. 15 shows a cross section of the distal portion of an inflow/outflow atraumatic sheath.

FIG. 16 shows a cross section of the distal portion of an inflow/outflow atraumatic sheath.

FIG. 17 shows an inflow/outflow atraumatic sheath for use with arthroscopic instruments.

FIG. 18 shows a cross section of the distal portion of the inflow/outflow sheath shown in FIG. 17.

FIG. 19 shows an inflow/outflow sheath having a distal portion that has an inner diameter that closely conforms to the outer diameter of the distal portion of an arthroscope.

### DETAILED DESCRIPTION OF THE INVENTIONS

FIG. 1 shows a method of performing arthroscopic surgery on a patient by using an arthroscopic instrument 2

3

sheathed in an atraumatic introducer sheath **3**. (The various parts of the arthroscope are shown in phantom to indicate their positions inside the sheath.) Various anatomical landmarks in the patient's knee **4** are shown for reference, including the femur **5**, patella **6**, posterior cruciate ligament **7**, anterior cruciate ligament **8**, meniscus **9**, tibia **10** and fibula **11**. During surgery, the surgeon introduces the arthroscope **2** into the knee via a first incision **12** in order to visualize the surgical field. A trimming instrument **13** is introduced through a second incision **14** to remove or trim tissue that the surgeon determines should be removed or trimmed. Optionally, an irrigating instrument **15** may be introduced through a third incision **16** in order to irrigate the surgical field and thereby maintain a clear view. As provided below, the irrigating instrument may be replaced by a combined arthroscope and inflow/outflow atraumatic sheath.

The arthroscope **2** is an optical instrument **17** surrounded by a rigid cannula **18** having a distal edge that typically is cut at an angle. To protect the patient from unintended injury or trauma during the procedure, the arthroscope has been inserted into a resilient, outer introducer sheath or atraumatic sheath **3** that extends over the rigid cannula. The distal tip **19** of the atraumatic sheath extends distally just past the distal end of the arthroscope and rigid cannula to further protect the patient.

FIGS. **2** through **4** illustrate the atraumatic sheath **3**. The atraumatic sheath is a tube of a resilient material, such as a soft plastic or rubber. The inner diameter of the atraumatic sheath is sized and dimensioned to closely fit over the outer diameter of an arthroscopic instrument. The distal tip **19** of the atraumatic sheath is provided with a shape that closely approximates the shape of the distal tip of the arthroscope and/or the rigid cannula. A flange **30** disposed around the distal end of the sheath prevents the distal tip of the rigid cannula from gouging the patient. The flange is integral with the walls of the sheath and extends inwardly towards the axis of the sheath. The flange is sized and dimensioned to prevent the distal tip of the rigid cannula from accidentally slipping distally during a surgical procedure. An opening **36** is provided in some atraumatic sheaths so that the surgeon may insert the endoscope or other instruments through the opening and into the surgical space. The distal lens **31** of an optical instrument is shown for reference in FIGS. **3** and **4**.

The proximal end **32** of the atraumatic sheath is provided with a tab **33** to allow medical personnel to easily pull the atraumatic sheath over the rigid cannula, arthroscope and/or arthroscopic instrument. The proximal end of the atraumatic sheath may also be provided with fittings **38**, such as a locking hub or snap latches, that attach to fittings **39** or openings disposed on the arthroscope or other instrument, thereby securing the atraumatic sheath as illustrated in FIG. **7**.

The outer surface of the atraumatic sheath may be provided with a smooth coating **40** as shown in FIG. **5** to allow the arthroscope and rigid cannula to more easily move within an operating site. For example, the sheath may be provided with a Teflon® (PTFE or expanded polytetrafluoroethylene) coating or covered with a water-activated lubricant. In contrast, the inner surface of the atraumatic sheath (the walls that define the lumen of the tube) may be provided with a non-slip coating **41** or other high coefficient of friction coating. For example, the inner surface of the atraumatic sheath may be coated with a co-extruded tacky thermoplastic elastomer (TPE). The non-slip coating prevents the sheath from easily slipping over the outer surface

4

of the rigid cannula or arthroscope, thereby helping to prevent the atraumatic sheath from twisting or slipping around the arthroscope.

FIGS. **3** and **4** show an atraumatic sheath **3** for use with arthroscopic instruments and an endoscope or arthroscope **2** disposed inside the atraumatic sheath. The atraumatic sheath shown in FIG. **3** is provided with a balloon **34** on the distal portion of the sheath. (The balloon may be integrally formed with the sheath.) The balloon allows a surgeon to open a space within tissue, thereby dissecting the surgical field. The arthroscope may then be extended distally out of the opening **36** and the surgical space visualized. In addition, the distal end of the sheath may be provided with a distally projecting spoon or other distally projecting object to prop open a space in front of the arthroscope. The balloon and the distally projecting spoon thus provide a means for dissecting or retracting tissue to form a small surgical space.

FIG. **4** shows an atraumatic sheath **3** having a second, working tube **35**. The working tube allows irrigation, fiber optics, sutures, needles, probes or surgical tools through the lumen. The atraumatic sheath shown in FIG. **4** may be combined with the atraumatic sheath shown in FIG. **3** to provide an atraumatic sheath with both a balloon and a working tube.

FIG. **5** shows a cross section of the atraumatic sheath **3** shown in FIG. **2** and an arthroscopic instrument **2** disposed inside the sheath. The atraumatic sheath is provided with a tab **33** on the proximal end of the sheath in order to increase the ease of pulling the sheath over the arthroscope. The distal end of the sheath is provided with an opening **36** to allow light to pass between the arthroscope and the operating space and, optionally, to allow additional instruments to pass through or alongside the arthroscope and into the surgical field. The walls **37** of the sheath at the distal end **19** of the sheath are thicker than the rest of the sheath walls to form a flange **30** at the distal end of the sheath. (The flange may be a separate ring of material attached to the inside of the sheath.) The flange covers the sharp distal tip of the arthroscopic instrument and prevents the instrument from slipping distally through opening **36**. The rest of the walls of the atraumatic sheath are thin in order to minimize the overall thickness of the combined sheath and arthroscopic instrument.

In use, the atraumatic sheath is provided and pulled over an arthroscopic instrument. (The instrument may also be thought of as being inserted into the sheath.) The sheathed arthroscopic instrument is then inserted into the surgical site and the surgeon performs a medical procedure therein. If a balloon is provided, the balloon is used to dissect tissue so that the arthroscope may be extended distally out of the opening **36** and the surgical space visualized.

FIGS. **6** and **7** show an inflow/outflow atraumatic sheath **50** and an arthroscope **2** disposed inside the sheath. Like the sheath shown in FIG. **2**, the inflow/outflow atraumatic sheath **50** is formed of a resilient material that protects the patient from accidental injury should the arthroscope poke at or scrape along tissue. The sheath material may also be radiopaque. A preferred durometer hardness of the sheath material is in the range of about 40 Shore D to about 90 Shore D. In this hardness range the sheath is sufficiently resilient that the sheath protects the patient from accidental injury but is sufficiently hard to prevent the lumens within sheath from collapsing.

The inflow/outflow sheath **50** is a multi-lumen tube into which an arthroscope is inserted. Each lumen extends from the distal portion **51** of the sheath to the proximal portion **52** of the sheath. The proximal portion of the sheath is provided

5

with one or more fluid ports, such as first port **53** or second port **54**; one or more stopcocks **55** or fluid switches; one or more valves, such as an anti-backflow valve; a manifold **56**; or other means of controlling the flow of fluid inside the sheath. The distal portion **51** of the inflow/outflow sheath is provided with a plurality of holes **57**. Each hole communicates with one or more of the lumens inside the tube, thereby allowing fluid to flow between the surgical field and the lumens inside the sheath.

Prior to surgery, medical personnel or the device manufacturer inserts the arthroscope into the inflow/outflow atraumatic sheath and secures the sheath to the arthroscope via a set-screw, snap-on attachment, other releasable attachments or other means **58** for securing the sheath to the arthroscope. During use, a surgeon may cause a fluid, preferably saline, to flow from a fluid source **59**, through the arthroscope and into the surgical field, as shown by inflow arrows **60**. (The arthroscope is provided with one or more lumens, ports or working tubes that allow fluid to flow through the arthroscope and into the surgical field.) In turn, blood, other fluids and debris are drained from the surgical field through the holes **57**, as shown by outflow arrows **61**, and flow through one or more lumens in the sheath. The inflow of clear saline and the outflow of cloudy fluid and debris allow the surgeon to maintain a clear surgical field using a single instrument. In turn, this capability eliminates the need to use an irrigating instrument. Thus, the surgeon may have a clear field of view while using only a two-incision arthroscopic procedure.

FIG. **7** also shows that fluids are drained through the inflow/outflow atraumatic sheath by using a vacuum source **70** or gravity drain operatively attached to a fluid port, such as port **53**, connected to the sheath manifold **56**. Fluids are provided through the arthroscope **2** from a fluid source **59** (by using a pump or gravity feed) operatively attached to a fluid port, such as third port **72** or fourth port **73** connected to the arthroscope. Depending on the capabilities of the arthroscope and the surgeon's needs, the vacuum source and fluid source may be connected to different combinations of ports provided with the inflow/outflow sheath or the arthroscope. For example, the vacuum source may be attached to port **73** and the fluid source may be attached to port **72** on the inflow/outflow sheath. In this case, the surgeon may both introduce fluids into and drain fluids from the surgical site using only the inflow/outflow sheath. Thus, even if the arthroscope is incapable of introducing fluids to or draining fluids from the surgical site, the inflow/outflow sheath allows the surgeon to eliminate the need for the irrigation instrument. In any case, a pressure sensor, and flow rate control system and feedback control system may be provided to automatically monitor and control the rate of fluid flow into and out of the surgical site.

FIG. **8** shows a cross section of the distal portion of the inflow/outflow sheath **3** shown in FIG. **6**. The inflow/outflow sheath **50** has a central lumen **80**, bounded by inner wall **81**, through which the arthroscope is inserted. The sheath has four outer lumens, including a first outer lumen **82**, a second outer lumen **83**, a third outer lumen **84** and a fourth outer lumen **85** bounded by the inner wall **81**, the outer wall **86** and four relatively stiff ribs **87** that extend between the inner and outer walls and that run along the length of the sheath. The distal end of the sheath in the area of the outer lumens **82**, **83**, **84** and **85** is sealed closed and provided with a rounded shape to help prevent injury to the patient (the central lumen remains open to accommodate the arthroscopic instrument). Holes **57** or apertures disposed in the outer wall allow fluids to flow into or out of the outer

6

lumens. For example, lumens **82** and **84** could serve as passages through which fluids are introduced into the surgical site and lumens **83** and **85** could serve as passages through which fluids are drained from the surgical site. During another surgical procedure, all four lumens could be used to either drain or introduce fluids. Thus, the surgeon has the option of using the inflow/outflow atraumatic sheath in many different modes. (In addition, the sheath may be formed with more than or fewer than the four ribs shown, so long as at least one outer lumen remains open to fluid flow after the sheath and scope have been inserted into the surgical site.)

FIGS. **9** through **16** show cross sections of the distal portion of various inflow/outflow atraumatic sheaths. FIG. **9** shows an inflow/outflow sheath having a second set of inner lumens, including a first inner lumen **100**, a second inner lumen **101**, a third inner lumen **102** and a fourth inner lumen **103**. With this design, the surgeon can increase the rate of fluid exchange by using all of the inner lumens to introduce fluids into the surgical site and by using all of the outer lumens **82**, **83**, **84** and **85** to drain fluid from the surgical site (or visa versa).

FIG. **10** shows an inflow/outflow sheath **50** without an inner wall. Instead, the outer surface of the arthroscope **2** serves as the inner wall of the sheath once the arthroscope has been inserted into the sheath. The four, relatively stiff ribs **87** form a seal with the outer surface of the arthroscope, thereby creating the four outer lumens **82**, **83**, **84** and **85**. The ends of the ribs may be provided with elastic flanges **104** to enhance the seal made between the ribs and the arthroscope. This configuration reduces the overall size of the combined inflow/outflow sheath and arthroscope. (If the outer wall **86** is made of an elastomeric material, then the tube can stretch radially to accommodate a variety of sizes of arthroscopes.)

FIG. **11** shows an inflow/outflow atraumatic sheath **50** similar to that shown in FIG. **10**. The relatively hard ribs **87** are pleated, but still form a seal with the outer wall of the arthroscope **2**, thereby forming the outer lumens **82**, **83**, **84** and **85** once the arthroscope is inserted into the sheath. The sheath of FIG. **11** accommodates a variety of sizes of arthroscopes since the pleated ribs will bend to a degree necessary to accommodate larger sizes of arthroscopes, as shown in FIG. **12**.

FIG. **13** shows an inflow/outflow atraumatic sheath **50** similar to that shown in FIG. **11**. The ribs **87** of this sheath are elastic tubes that form a seal with the outer wall of the arthroscope **2**, thereby forming the outer lumens **82**, **83**, **84** and **85** once the arthroscope is inserted into the sheath. The sheath of FIG. **13** accommodates a variety of sizes of arthroscopes since the tubes will compress to a degree necessary to accommodate larger sizes of arthroscopes, as shown in FIG. **14**.

FIG. **15** shows a "C"-shaped or slit inflow/outflow sheath **50**. Like the sheath of FIG. **8**, four outer lumens **82**, **83**, **84** and **85** are provided, with the outer lumens bounded by three ribs **87**, the inner wall **81** and the outer wall **86**. When the arthroscope **2** is inserted into the sheath, a small gap **105** may form between the respective tips of the first arcuate segment **106** and the second arcuate segment **107**. (As the arthroscope is inserted into the surgical space, tissue **108** will seal the gap and prevent fluids from leaking from the surgical space to outside the body.) The sheath of FIG. **15** accommodates a variety of sizes of arthroscopes since the arcuate segments will move radially outwardly as a larger arthroscope is inserted into the sheath, as shown in FIG. **16**.

Optionally, a protrusion or a guide rail **109** may extend from either the arthroscope or the sheath. The guide rail

helps the user align the sheath on the arthroscope while inserting the arthroscope into the sheath. The guide rail also prevents unwanted rotation or twisting of the sheath over the arthroscope during a surgical procedure.

FIGS. 17 and 18 show an inflow/outflow atraumatic sheath 50 and an arthroscope 2 inserted into the sheath. In contrast to the inflow/outflow sheaths shown in FIGS. 6 through 16, the outer wall 86 of the distal portion 51 of the sheath is made from a continuous tube (the distal portion of the sheath is not provided with holes). Nevertheless, like the sheath of FIG. 8 the sheath of FIG. 17 has an inner lumen to accommodate the arthroscope and four outer lumens to accommodate fluid inflow and outflow, including a first outer lumen 82, a second outer lumen 83, a third outer lumen 84, and a fourth outer lumen 85. The outer lumens are bounded by the inner wall 81, outer wall 86 and supporting ribs 87. The instrument shown in FIG. 17 provides fluid inflow and outflow out of the distal end 110 of the sheath.

FIG. 19 shows an inflow/outflow atraumatic sheath 50 having a closely-conforming distal portion 111 that has an inner diameter that closely conforms to the outer diameter of the distal portion of an arthroscope 2. The fluid-conducting portion 112 of the sheath is set proximally from the closely conforming distal portion 111 of the sheath. The outer diameter of the fluid conducting portion 112 and the outer diameter of the closely conforming distal portion 111 may be formed integrally with each other such that both portions are part of the same sheath. Holes 57 disposed in the fluid-conducting portion 112 just proximally of the distal portion 111 of the sheath communicate with one or more lumens inside the sheath, thereby allowing a surgeon to either introduce or drain fluids from a surgical site. The sheath shown in FIG. 19 has a distal portion 111 with a relatively small radius, since the sheath closely conforms to the arthroscope at the distal portion of the arthroscope. This provides the surgeon with the capability of inserting the arthroscope into narrow surgical sites. In addition, the fluid-conduction portion still allows a surgeon to irrigate the surgical field with the combined sheath/arthroscope instrument.

Since the atraumatic sheath may be designed or sized and dimensioned to conform to differently shaped instruments, the sheath is also useful with other medical instruments and other surgical procedures in which it is desirable to protect surrounding tissue from accidental trauma. For example, the atraumatic sheath may be disposed over a trimming instrument for use during arthroscopic surgery or over an energy-delivering medical instrument, such as a laser or RF energy instrument. Other procedures in which the atraumatic sheath is useful include laparoscopic surgery and other kinds of endoscopic surgery. In addition, the various sheath configurations shown herein may be combined to form additional types of instrument sheaths. Thus, while the preferred embodiments of the devices and methods have been described in reference to the environment in which they were developed, they are merely illustrative of the principles of the inventions. Other embodiments and configurations may be devised without departing from the spirit of the inventions and the scope of the appended claims.

We claim:

1. A system for performing arthroscopic surgery, said system comprising:

an arthroscopic instrument suitable for performing an arthroscopic surgical procedure, said arthroscopic instrument characterized by a distal tip;

a rigid cannula, said rigid cannula characterized by a lumen and a distal tip, said rigid cannula sized and

dimensioned such that the arthroscopic instrument may be extended through the lumen and distally of the distal tip of the rigid cannula;

an atraumatic sheath comprising a tube of resilient material having a distal end, said sheath having an opening at the distal end of the sheath, said sheath having an inner diameter sized and dimensioned to closely conform to an outer diameter of the rigid cannula, said sheath having an interior surface;

a ring secured to the interior surface of the sheath at the distal end of the sheath, said ring disposed, sized and dimensioned to prevent the distal tip of the rigid cannula from extending distally from the sheath, said ring disposed, sized and dimensioned to allow the arthroscopic instrument to extend distally from the distal end of the sheath;

wherein the atraumatic sheath is adapted to be removably disposed over the arthroscopic instrument.

2. The system of claim 1 wherein the sheath is provided with a tab disposed on the proximal end of the sheath, said tab sized and dimensioned to allow the sheath to be pulled onto and off of the arthroscopic instrument.

3. The system of claim 1 further comprising a first set of fittings disposed on the proximal end of the sheath and a second set of fittings disposed on the arthroscopic instrument, wherein the first and second sets of fittings are adapted for releasable coupling, whereby the sheath is secured to the arthroscopic instrument when the first and second sets of fittings are secured together.

4. The system of claim 1 wherein the atraumatic sheath is characterized by a distal portion and wherein the atraumatic sheath further comprises a balloon disposed on the distal portion of the sheath.

5. The system of claim 1 wherein the sheath further comprises a working tube, said working tube sized, dimensioned and disposed to allow fluid communication between a surgical site and the lumen of the working tube.

6. The system of claim 1 wherein the sheath further comprising a balloon disposed on the distal portion of the sheath, said sheath further comprising a working tube, said working tube sized, dimensioned and disposed to allow fluid communication between a surgical site and the lumen of the working tube.

7. A method of performing arthroscopic surgery, said method comprising the steps of:

providing a system for performing arthroscopic surgery, said system comprising:

an arthroscopic instrument suitable for performing an arthroscopic surgical procedure, said arthroscopic instrument characterized by a distal tip;

a rigid cannula, said rigid cannula characterized by a lumen and a distal tip, said rigid cannula sized and dimensioned such that the arthroscopic instrument may be extended through the lumen and distally of the distal tip of the rigid cannula;

an atraumatic sheath comprising a tube of resilient material having a distal end, said sheath having an opening at the distal end of the sheath, said sheath having an inner diameter sized and dimensioned to closely conform to an outer diameter of the rigid cannula, said sheath having an interior surface;

a ring secured to the interior surface of the sheath at the distal end of the sheath, said ring disposed, sized and dimensioned to prevent the distal tip of the rigid cannula from extending distally from the sheath, said

9

ring disposed, sized and dimensioned to allow the arthroscopic instrument to extend distally from the distal end of the sheath;

wherein the atraumatic sheath is adapted to be removably disposed over the arthroscopic instrument; 5 placing the arthroscopic instrument inside of the rigid cannula;

placing the rigid cannula inside of the atraumatic sheath; performing an arthroscopic surgical procedure.

8. The method of claim 7 wherein the sheath is provided with a tab disposed on the proximal end of the sheath, said tab sized and dimensioned to allow the sheath to be pulled onto and off of the arthroscopic instrument. 10

9. The method of claim 7 further comprising a first set of fittings disposed on the proximal end of the sheath and a second set of fittings disposed on the arthroscopic instrument, wherein the first and second sets of fittings are adapted for releasable coupling, whereby the sheath is secured to the arthroscopic instrument when the first and second sets of fittings are secured together. 15

10. The method of claim 7 wherein the atraumatic sheath is characterized by a distal portion and wherein the atraumatic sheath further comprises a balloon disposed on the distal portion of the sheath. 20

11. The method of claim 7 wherein the sheath further comprises a working tube, said working tube sized, dimensioned and disposed to allow fluid communication between a surgical site and the lumen of the working tube. 25

12. The method of claim 7 wherein the sheath further comprising a balloon disposed on the distal portion of the sheath, said sheath further comprising a working tube, said working tube sized, dimensioned and disposed to allow fluid communication between a surgical site and the lumen of the working tube. 30

13. A system for performing arthroscopic surgery, said system comprising: 35

an optical instrument suitable for performing an arthroscopic surgical procedure, said optical instrument characterized by a distal tip;

a rigid cannula, said rigid cannula characterized by a lumen and a distal tip, said rigid cannula sized and dimensioned such that the optical instrument may be extended through the lumen and distally of the distal tip of the rigid cannula; 40

10

an atraumatic sheath comprising a tube of resilient material having a distal end, said sheath having an opening at the distal end of the sheath, said sheath having an inner diameter sized and dimensioned to closely conform to an outer diameter of the rigid cannula, said sheath having an interior surface;

a ring secured to the interior surface of the sheath at the distal end of the sheath, said ring disposed, sized and dimensioned to prevent the distal tip of the rigid cannula from extending distally from the sheath, said ring disposed, sized and dimensioned to allow the optical instrument to extend distally from the distal end of the sheath;

wherein the atraumatic sheath is adapted to be removably disposed over the optical instrument.

14. The system of claim 13 wherein the sheath is provided with a tab disposed on the proximal end of the sheath, said tab sized and dimensioned to allow the sheath to be pulled onto and off of the optical instrument. 20

15. The system of claim 13 further comprising a first set of fittings disposed on the proximal end of the sheath and a second set of fittings disposed on the optical instrument, wherein the first and second sets of fittings are adapted for releasable coupling, whereby the sheath is secured to the optical instrument when the first and second sets of fittings are secured together.

16. The system of claim 13 wherein the atraumatic sheath is characterized by a distal portion and wherein the atraumatic sheath further comprises a balloon disposed on the distal portion of the sheath.

17. The system of claim 13 wherein the sheath further comprises a working tube, said working tube sized, dimensioned and disposed to allow fluid communication between a surgical site and the lumen of the working tube.

18. The system of claim 13 wherein the sheath further comprising a balloon disposed on the distal portion of the sheath, said sheath further comprising a working tube, said working tube sized, dimensioned and disposed to allow fluid communication between a surgical site and the lumen of the working tube.

\* \* \* \* \*